

Measurement Data Recognition from Seven-Segment Indicator by Mobile Device



Ivan Timofeev, YarSU

Use Case





Make sure that measurement values are inside the selection area and wait until recognition is done.



The 'Edit' screen in the mobile app shows the following data:



Field	Value
Systolic	126
Diastolic	78
Heart rate	61
Date	16/04/2014
Time	19:50

At the bottom, there are 'Save' and 'Cancel' buttons. A text area labeled 'Make a note here' is also present.

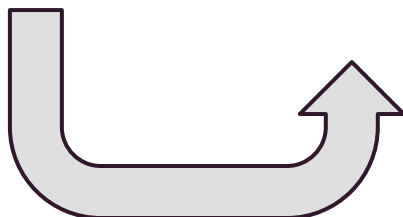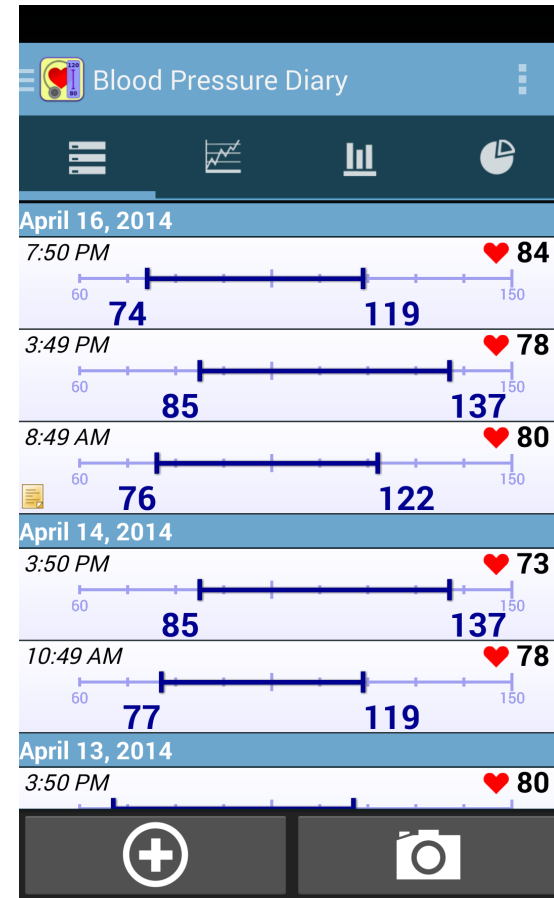




Blood Pressure Diary

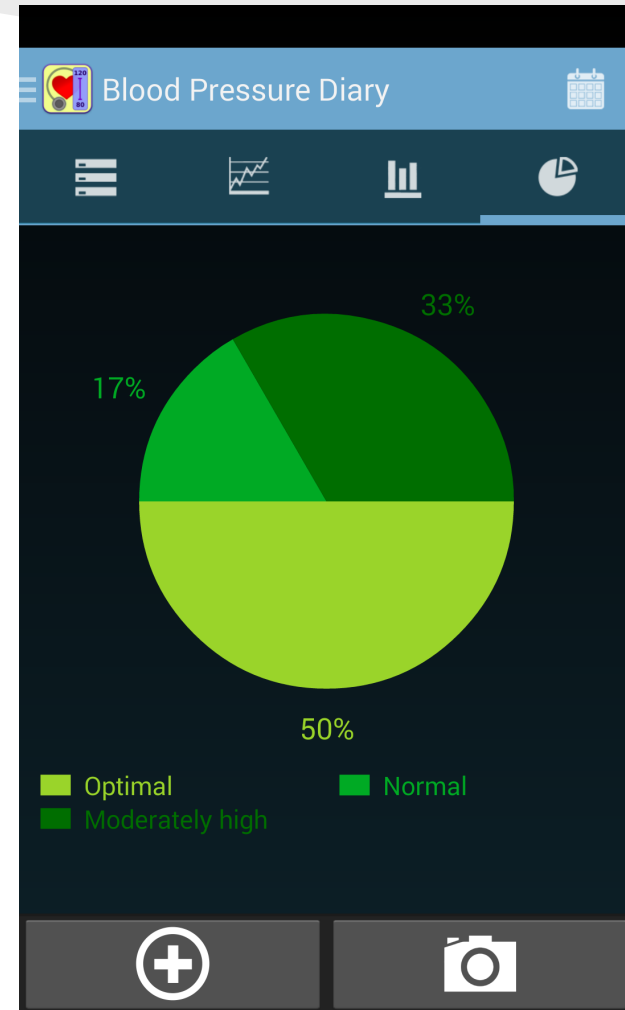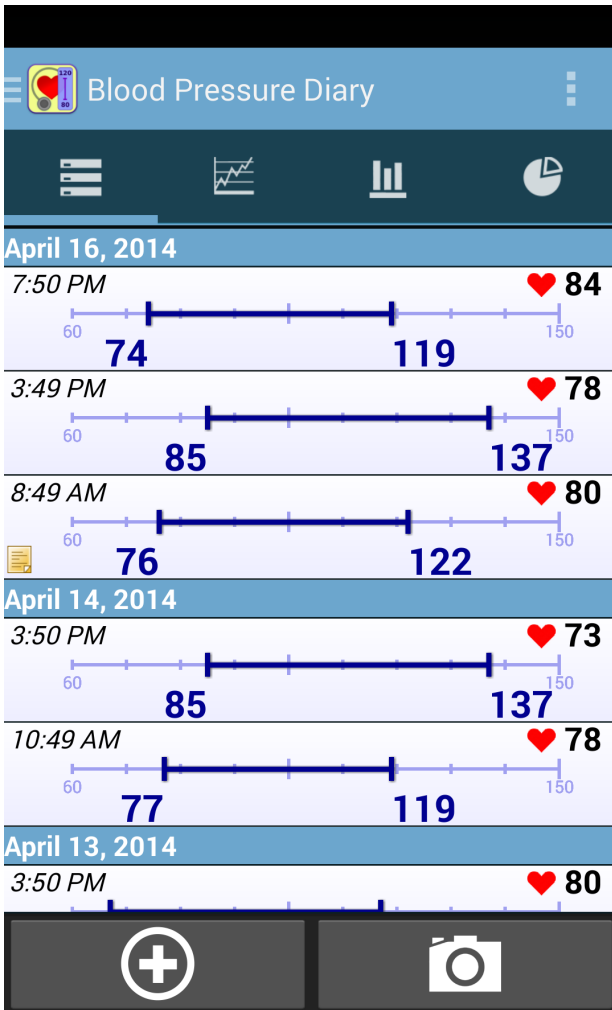



NFC

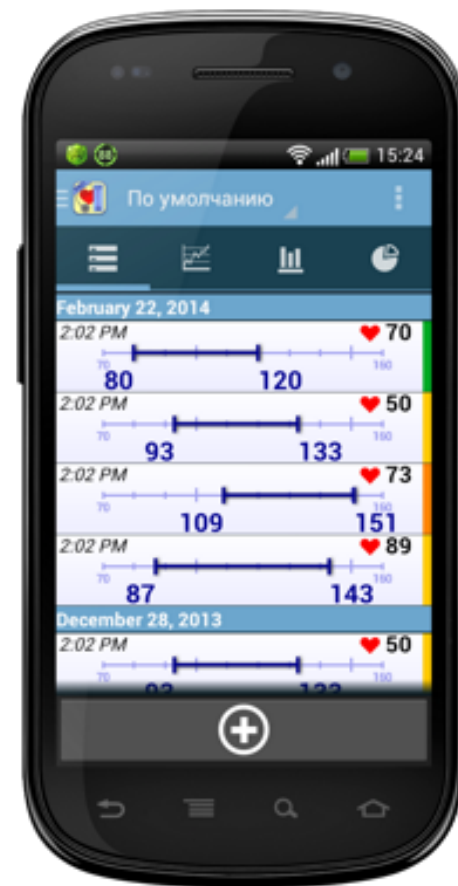

Blood Pressure Diary

**Welcome
to our stand!**

